

LAB STANDARDS

DEVICE	PLATE MATERIAL*	HEEL CUP DEPTH	DEVICE WIDTH	DEVICE LENGTH	EXTENSION LENGTH	REARFOOT POSTING**	TOP COVER
Functional	Poly/3D	12mm	Standard	To mets	To mets	Extrinsic to vertical	Leatherette
Dress	Poly/3D	8mm	Hourglass	To mets	To mets	Intrinsic to vertical	Leatherette
Accommodative	Cork	12mm	Standard	To toes	To toes	Intrinsic to vertical	P-cell

*Plate thickness chosen according to patient weight. Please refer to weight chart. **Forefoot posting standard is intrinsic to cast.


ACCOMMODATIONS

Medial Flange	Medium
Medial Heel Skive (Kirby Skive)	4mm
Heel Lift	Crepe
Runner's Wedge	3 degree crepe
Arch Reinforcement	Poron
Padded Heel	Soft, 1/8" Poron
Horseshoe Pad	Soft, 1/8" Poron
Scaphoid Pad	Soft, 1/8" Poron
Soft Flange	Soft, 1/8" Poron
Toe Crest	Soft, 1/8" Poron
Cutout	Thickness of padding
Channel	Thickness of padding
Balance Pad	Soft, 1/8" Poron
Morton's Extension	Firm, 1/8" Duraform
Dancer's Pad	Soft, 1/8" Poron


ORTHOTIC PADDING MATERIAL

Material	Soft, Poron
Thickness	1/8"
Length	To mets

Arch Height

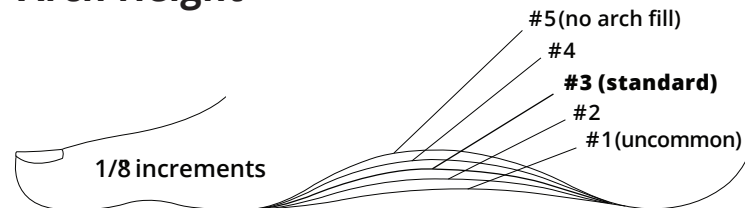

Shell Width

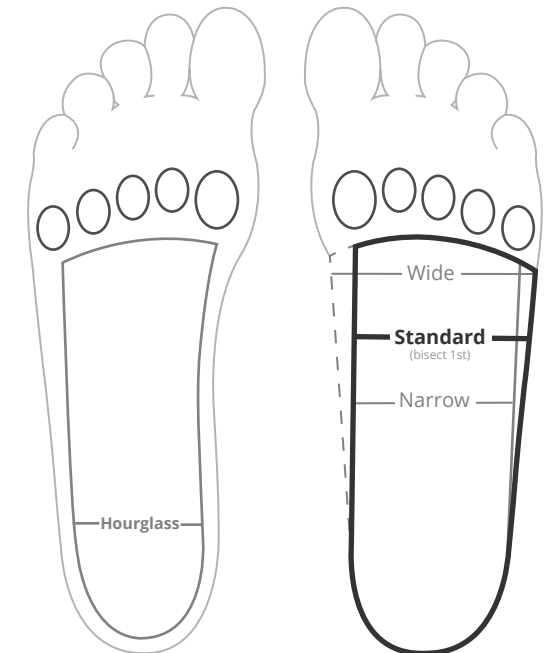

Completing order forms significantly reduces lab questions, expediting orders into production.
Should any section be left blank, Lab Standards will be used.

REVISED 3/8/2021 (F)

SOLO Laboratories, Inc. • 415 South Laurel Street, Kutztown, PA 19530 • 800.765.6522 • Fax 610.683.6427 • info@sololabs.com • www.sololabs.com

SOLO[®]