

LAB STANDARDS

DEVICE	PLATE MATERIAL*	HEEL CUP DEPTH	DEVICE WIDTH	DEVICE LENGTH	EXTENSION LENGTH	REARFOOT POSTING**	TOP COVER
Functional	Poly / 3D PA12	12mm	Standard	To mets	To mets	Extrinsic to vertical	Leatherette
Dress	Poly / 3D PA12	8mm	Hourglass	To mets	To mets	Intrinsic to vertical	Leatherette
Accommodative	Cork	12mm	Standard	To toes	To toes	Intrinsic to vertical	P-cell

*Plate thickness chosen according to patient weight. Please refer to weight chart. Default plate material is 3D PA12 when possible. **Forefoot posting standard is intrinsic to cast.


ACCOMMODATIONS

Medial Flange	Medium
Medial Heel Skive (Kirby Skive)	4mm
Heel Lift	Crepe
Runner's Wedge	3 degree crepe
Arch Reinforcement	Poron
Padded Heel	Soft, 1/8" Poron
Horseshoe Pad	Soft, 1/8" Poron
Met Pad / Bar	Soft, 1/8" Poron
Scaphoid Pad	Soft, 1/8" Poron
Soft Flange	Soft, 1/8" Poron
Toe Crest	Soft, 1/8" Poron
Cutout	Thickness of padding
Channel	Thickness of padding
Balance Pad	Soft, 1/8" Poron
Morton's Extension	Firm, 1/8" Duraform
Dancer's Pad	Soft, 1/8" Poron


ORTHOTIC PADDING MATERIAL

Material	Soft, Poron
Thickness	1/8"
Length	To mets

Arch Height

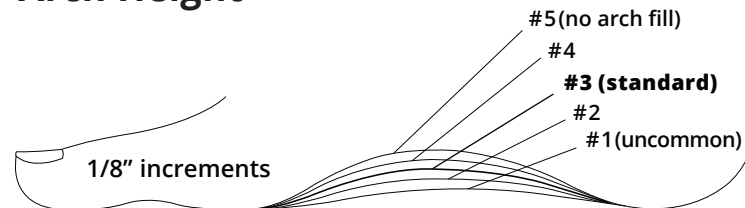

Shell Width

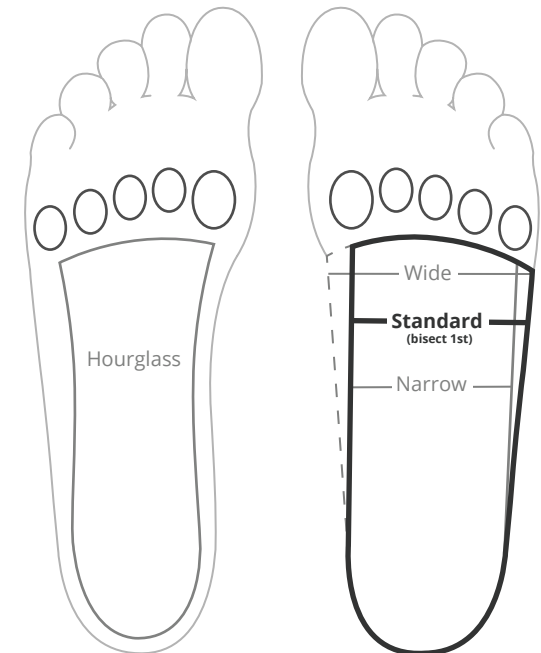

Completing order forms significantly reduces lab questions, expediting orders into production. Should any section be left blank, Lab Standards will be used.

REVISED 2022-05-17