LAB STANDARDS

DEVICE	PLATE MATERIAL*	HEEL CUP DEPTH	DEVICE WIDTH	DEVICE LENGTH	EXTENSION LENGTH	REARFOOT POSTING**	TOP COVER
Functional and Limited	3D-B Printed or 1/8" Poly	12mm	Standard	To mets	To mets	Extrinsic to vertical	Leatherette
Dress	3D-B Printed or 1/8" Poly	8mm	Hourglass	To mets	To mets	Intrinsic to vertical	Leatherette
Accommodative	Cork	12mm	Standard	To toes	To toes	Intrinsic to vertical	P-cell

^{*}Plate thickness chosen according to patient weight. Please refer to weight chart. If weight not given, thickness will be chosen as shown above. Default plate material is 3D printed when possible.

ACCOMMODATIONS

Medial Flange	Medium		
Medial Heel Skive (Kirby Skive)	4mm		
Heel Lift	Crepe		

Runner's Wedge 3 degree crepe

Arch Reinforcement Soft
Padded Heel Soft, 1/8"
Horseshoe Pad Soft, 1/8"
Scaphoid Pad Soft, 1/8"
Soft Flange Soft, 1/8"
Toe Crest Soft, 1/8"

CutoutThickness of paddingChannelThickness of padding


Balance Pad Soft, 1/8" Morton's Extension Firm, 1/8" Dancer's Pad Soft, 1/8"

ORTHOTIC PADDING MATERIAL

MaterialSoftThickness1/8"LengthTo mets

#5(no arch fill) #4 #3 (standard) #2 #1(uncommon)

Shell Width

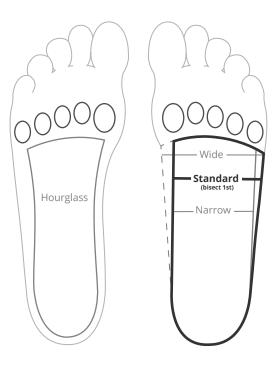

Completing order forms significantly reduces lab questions, expediting orders into production. Should any section be left blank, Lab Standards will be used.

REVISED 2025-04-09



^{**}Forefoot posting standard is intrinsic to cast.